


Tue Feb 24 08:34:36 2004


TIDE Mass_0

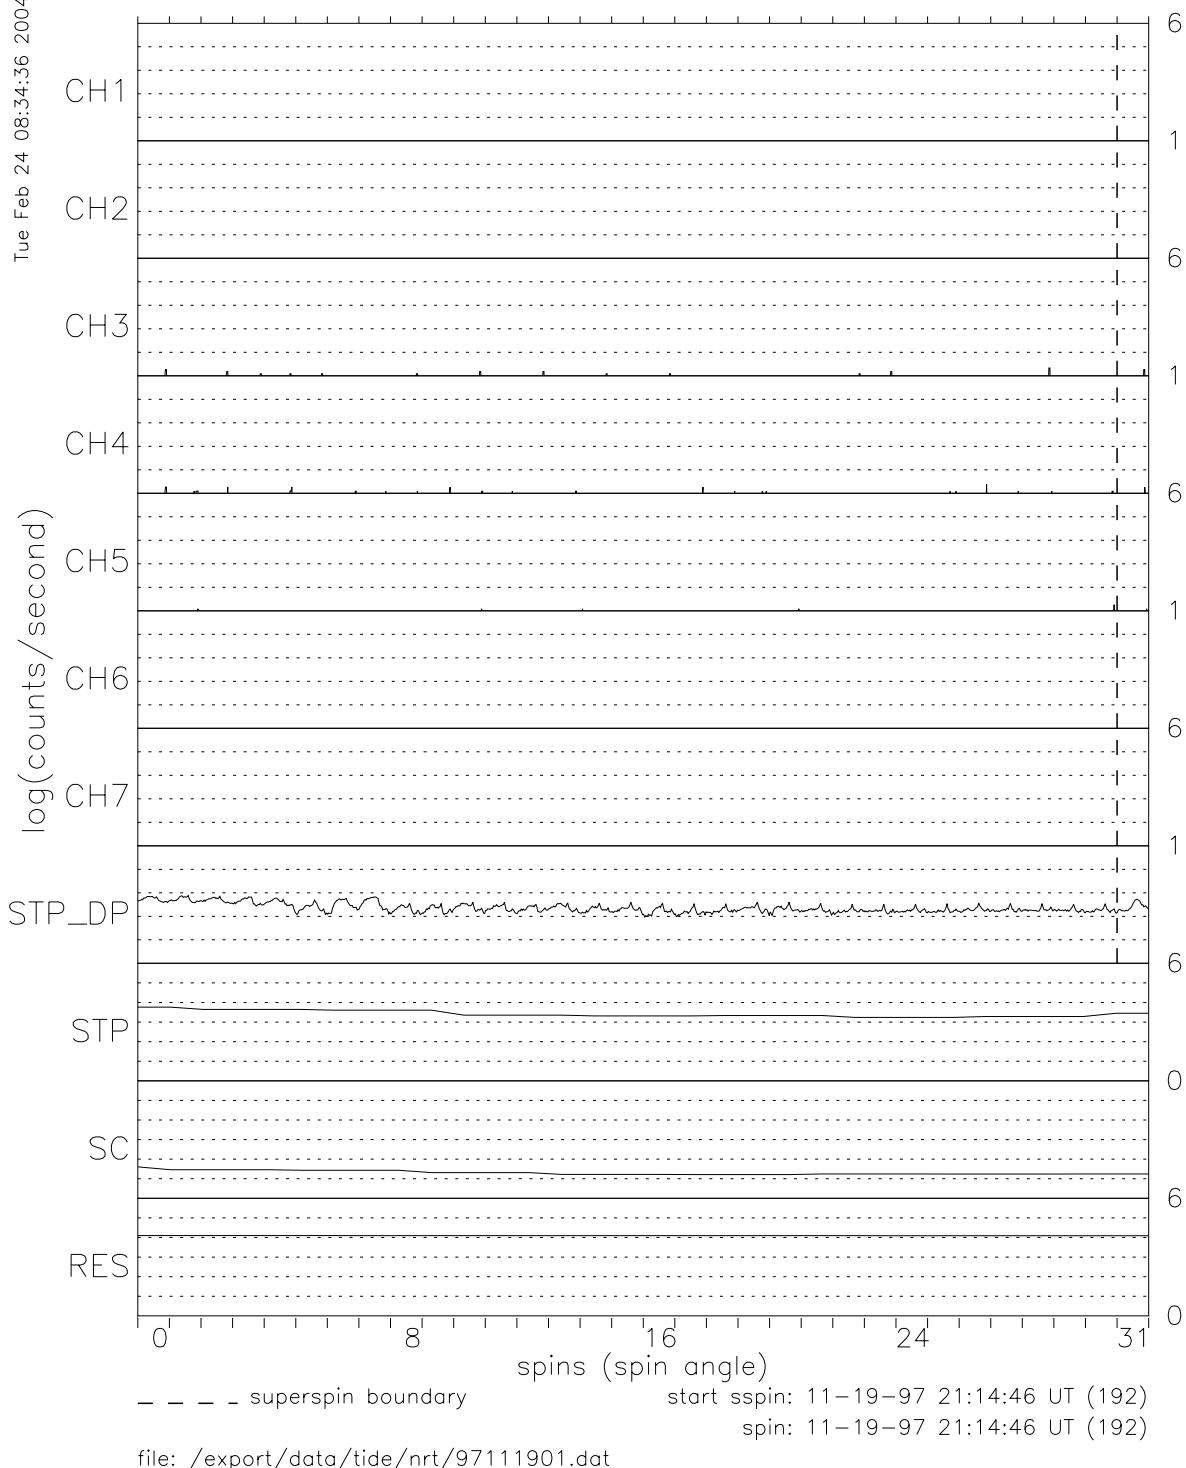

-15kV TOF: -9245 v
-3.6kV MCP: -2578 v
-2.4kV MCP: -1589 v
Input Cur: 302 ma
RPA max: 237 v
Mirror max: 238 v

Tue Feb 24 08:34:36 2004

TIDE Direct Events

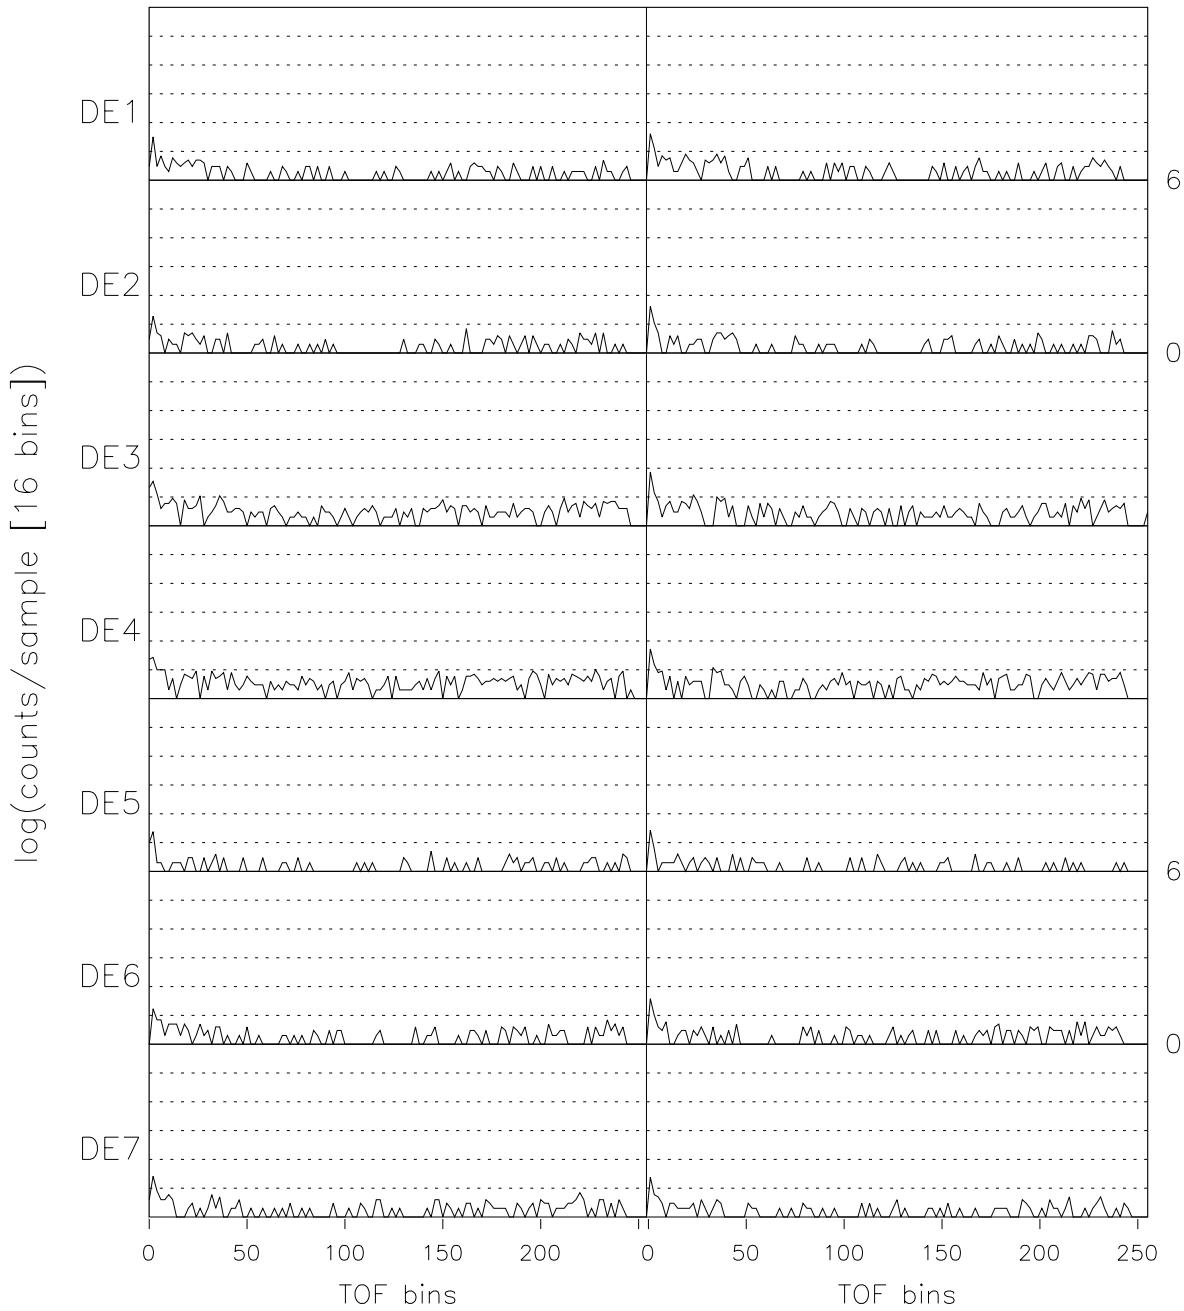

reported: 11-19-97 21:08:15 UT

reported: 11-19-97 21:11:28 UT

file: /export/data/tide/nrt/97111901.dat

-15kV TOF: -9116 v

-3.6kV MCP: -2593 v

-2.4kV MCP: -1579 v

Input Cur: 304 ma

RPA max: 237 v

Mirror max: 238 v